


**DIGITAL-TO-ANALOGUE  
METER WITH A MULTICOLOUR  
BARGRAPH  
+ SERIAL INTERFACE  
NA3 TYPE**



**USER'S GUIDE**



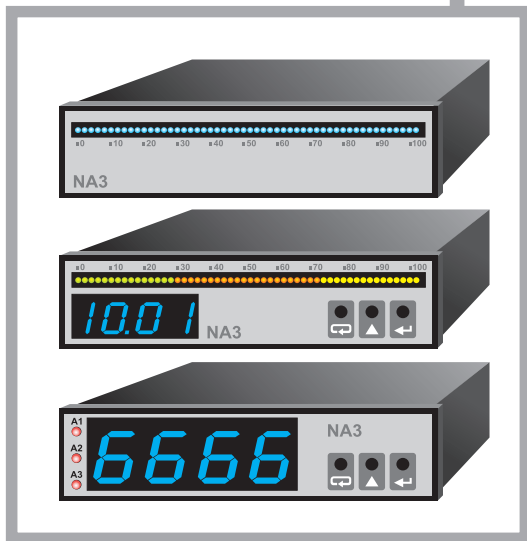

# **DIGITAL-TO-ANALOGUE METER WITH A MULTICOLOUR BARGRAPH + SERIAL INTERFACE NA3 TYPE**

<b>CONTENTS</b>	<b>Page</b>
1. APPLICATION .....	5
2. SET OF THE METER .....	6
3. BASIC REQUIREMENTS, OPERATIONAL SAFETY .....	7
4. INSTALLATION .....	9
5. SERVICING .....	11
6. RS-485 INTERFACE .....	28
7. TECHNICAL DATA .....	45
8. BEFORE A FAILURE HAS BEEN DECLARED .....	49
9. EXAMPLES OF NA3 METER PROGRAMMING .....	50
10. ORDERING PROCEDURE .....	52
11. MAINTENANCE AND GUARANTEE .....	56



## 1. APPLICATION

NA3 series meters with a multicoloured bargraph have an universal input destined to measure temperature, resistance, voltage from shunts, standard signals, d.c. voltage and d.c. current.

NA3 meters can optionally have a continuous analogue output, relays, OC type (Open Collector) and digital RS-485 outputs.

They can find application in various industrial fields, e.g. food industry, intermediate pumping stations, sewage treatment plants, chemical industry, weather stations, breweries.

NA3 meters are executed in three basic versions:

- NA3-F with a 4-digit LED readout field (digit height: 7 mm) and a multicolour bargraph,
- NA3-D with a 4-digit LED readout field (digit height: 14 mm),
- NA3-B with a multicolour bargraph.

The type choice is made in the execution code.

They are programmed by means of the keyboard and through RS-485. Meters only with the bargraph can be programmed through RS-485.

NA3 meters realise following functions:

- measurement of the input quantity and displaying it on the display and/or the bargraph,
- evaluation of the input signal into indication on the base of the individual linear characteristic,
- programming of the colour and bargraph resolutions (no concerns NA3-D),
- signalling of alarm value setting exceeding,
- recording of the measured signal in programmed time segments,
- storage of maximal and minimal values,
- programming of the indication resolution,
- programming of the measurement averaging time,
- locking of the parameter introduction by means of a password,
- conversion of the measured quantity into a voltage or current output signal,
- service of the RS-485 interface in MODBUS protocol, both in ASCII and RTU mode.



**Fig.1. View of the NA3 meter: a) NA3-F, b) NA3-D, c) NA3-B**

## 2. SET OF THE NA3 METER

We deliver in the set:

- NA3 meter ..... 1 pc.
- user's guide..... 1 pc.
- guarantee card ..... 1 pc.
- plug with screw terminals ..... 1 pc
- holders to fix the indicator in the panel..... 2 pcs
- set of stickers with units ..... 1 pc.

***When unpacking the meter, please check whether the type and execution code on the data plate correspond to the order.***

### 3. BASIC REQUIREMENTS, SAFETY INFORMATION

Symbols located in this service manual mean:

#### **WARNING!**



Warning of potential, hazardous situations. Especially important. One must acquaint with this before connecting the NA3 meter. The non-observance of notices marked by these symbols can occasion severe injuries of the personnel and the damage of the instrument.

#### **CAUTION!**



Designates a general useful note. If you observe it, handling of the meter is made easier. One must take note of this when the instrument is working inconsistently to the expectations.

#### **Possible consequences if disregarded !**

In the security scope the NA3 meter meets the requirements of the EEC Low-Voltage directive (EN 61010 -1 issued by CENELEC).

#### **Remarks concerning the operator safety:**



##### **1. General**

- The NA3 meter is destined to be mounted on a panel.
- Non-authorized removal of the required housing, inappropriate use, incorrect installation or operation creates the risk of injury to personnel or damage to equipment. For more detailed information please see the user's guide.
- All operations concerning transport, installation, and commissioning as well as maintenance must be carried out by qualified, skilled personnel and national regulations for the prevention of accidents must be observed.
- According to this basic safety information, qualified, skilled personnel are persons who are familiar with the installation, assembly, commissioning, and operation of the product and who have qualifications necessary for their occupation.

##### **2. Transport, storage**

Please observe the notes on transport, storage and appropriate handling. Observe the climatic conditions given in Technical Data.

##### **3. Installation**

- The NA3 meter must be installed according to the regulation and instructions given in this service manual.
- Ensure proper handling and avoid mechanical stress.

- Do not bend any components and do not change any insulation distances.
- Do not touch any electronic components and contacts.
- Instruments may contain electrostatically sensitive components, which can easily be damaged by inappropriate handling.
- Do not damage or destroy any electrical components since this might endanger your health!

#### **4. Electrical connection**

- Before switching the meter on, one must check the correctness of connection to the network.
- In case of the protection terminal connection with a separate lead one must remember to connect it before the connection of the instrument to the mains.
- When working on live instruments, the applicable national regulations for the prevention of accidents must be observed.
- The electrical installation must be carried out according to the appropriate regulations (cable cross-sections, fuses, PE connection). Additional information can be obtained from the user's guide.
- The documentation contains information about installation in compliance with EMC (shielding, grounding, filters and cables). These notes must be observed for all CE-marked products.
- The manufacturer of the measuring system or installed devices is responsible for the compliance with the required limit values demanded by the EMC legislation.

#### **5. Operation**

- Measuring systems including NA3 meters must be equipped with protection devices according to the corresponding standard and regulations for prevention of accidents.
- After the instrument has been disconnected from the supply voltage, live components and power connections must not be touched immediately because capacitors can be charged.
- The housing and the door must be closed during operation.

#### **6. Maintenance and servicing**

Please observe the manufacturer's documentation.

Read all product-specific safety and application notes in this user's guide manual

- Before taking the meter housing out, one must turn the supply off.
- The removal of the instrument housing during the guarantee contract period may cause its cancellation.



## 4. INSTALLATION

### 4.1. Fitting

Prepare a ( $22.2^{+0.5} \times 92^{+0.5}$ ) mm hole in the panel. The thickness of the material from which the panel is made should be in the range 1...15 mm.


The meter has screw terminal strips which enable the connection of 2.5 mm<sup>2</sup> cross-section external conductors.

Meter dimensions are shown on the fig. 2.

### 4.2. External connection diagrams

The description of terminal strips are shown on the fig. 3a.


Taking into consideration electromagnetic interference it is recommended to use

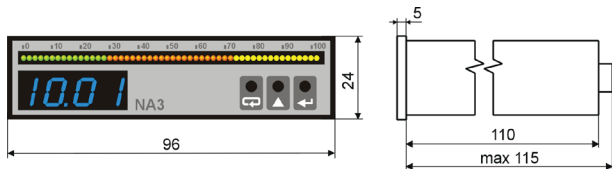


**Fig. 2. Meter overall dimension**

shielded conductors for the connection of input and output signals.


The power supply must be connected by means of a two-wire conductor with a suitable cross-section ensuring its protection by means of a fuse element.

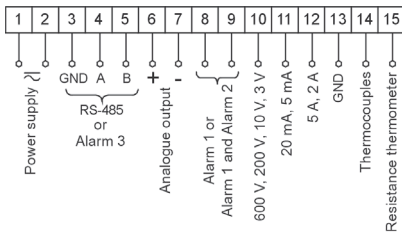


**a/ Description of the terminal strip**

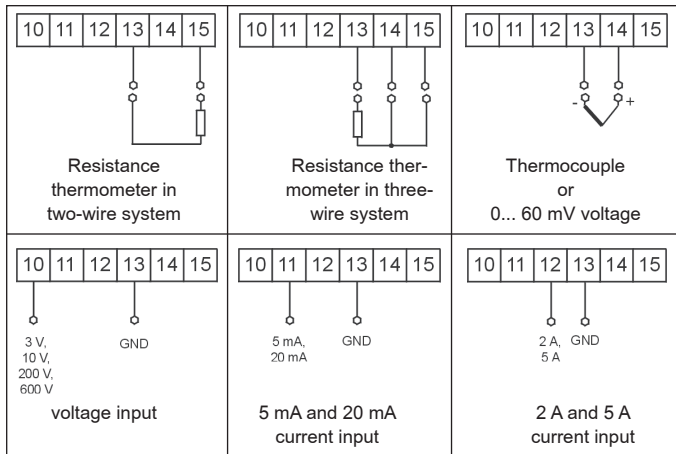

**b/ Connection way of input signals**

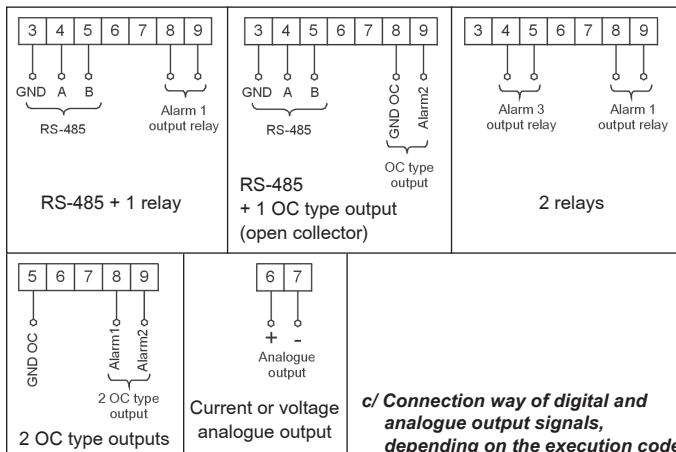

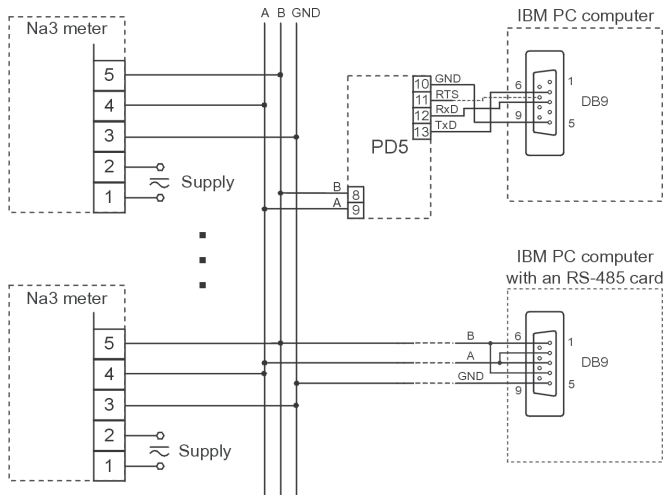

**d/ Connection way of the RS-485 interface**

**Fig.3 External connections of the NA3 meter**

Requirements concerning the power supply cable are regulated by EN 61010-1 p. 6.10. standard.

## 5. SERVICING

After connecting external signals and switching the meter on, its name *NA-3* and also the current version of the program, e.g. *v 100* are displayed.


After ca 3 seconds, the meter is transiting automatically into the working mode in which it carries out the measurement and the display of the measured value on the display and the bargraph. Depending on alarm and bargraph parameter settings, alarm thresholds are also displayed on the bargraph. The meter blanks automatically insignificant zeros.

### Key functions:



- acceptance key

- entry into the programming mode (hold down during ca 3 seconds),
- entry into the chosen parameter level,

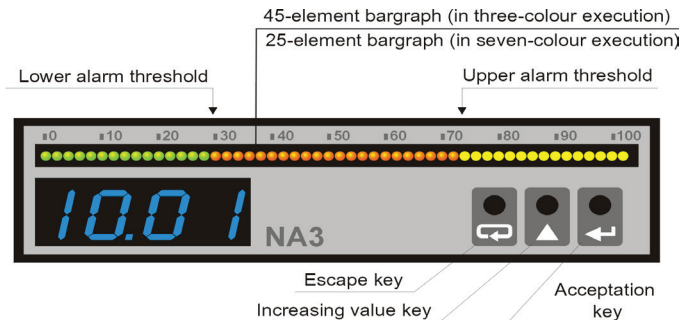

**Fig. 4 Description of the NA3F and NA3D frontal plate.**

- entry into the changing mode of the parameter value,
- acceptance of the changed parameter value.




- Key to increase the value




- display of the minimal value (first pressure), maximal (second pressure), return to measurement (third pressure),
- moving on the preview menu or programming matrix,
- change of the chosen parameter value - increasing of the value.







- Escape key

- entry into the menu of parameter preview (hold down ca 3 seconds),
- exit from the preview menu or programming matrix,
- escape from the parameter change.

The pressure and hold down the  key during 3 seconds causes the entry into the programming mode. The programming mode is protected by the *SE* safety code.

The pressure and hold down the  key during 3 seconds causes the entry into the preview menu. One must move on the preview menu by means of the  key. In this menu, only all programmed parameters, except servicing parameters, are accessible to readout. The exit from the preview menu is operated by means of the  key.

In the preview menu, it is also possible to review recorded *rESL* values. The pressure of the  key on the *rESL* parameter causes the entry into the preview menu of recorded values. The number of the recorded result is displayed alternately with the value e.g.  $n320/2174$ . The moving on recorded values takes place by means of the  key. The hold down of this key longer than ca 2 seconds will cause the acceleration of the review. The pressure of the  key in any time will cause the display of the number of recorded results. The exit from the review of recorded values is operated by means of the  key.

The algorithm of the meter servicing is presented on the fig. 5.

The appearance of the following symbols and inscriptions on the display means: It is possible to change meter parameters:

- from the meter keyboard (only in NA3-F and NA3-D executions) ..... - p. 5.1
- through RS-485 ..... - p.6.

### 5.1. Change of the NA3 meter parameters from the keyboard



Incorrectly introduced safety code



Exceeding of the upper measuring range or lack of sensor







Exceeding of the lower measuring range or short-circuited sensor





Error of the conductor resistance compensation.  
No connected conductor or damaged conductor.



The pressure of the  key during ca three seconds causes the display of the **SEI** inscription alternately with the set value 0 by the manufacturer. The introduction of the correct code causes the entry into the programming mode. The fig.6 represents the transition matrix into the programming mode. One can move on groups of main parameters eg: **Chn, bAr1, AI1, AI2**, etc, by means of the  key.

The pressure of the  key on the given level, causes the entry into parameters of this level. The moving on the given level is operated by means of the  key.

In order to change the value, one must use the  key. In order to escape from the parameter change, one must press the  key.

By means of the  key, one can exit from the selected level and programming matrix to the measurement.

During the meter operation in the programming mode the measurement result is displayed on the bargraph, except the selection of the display testing function.

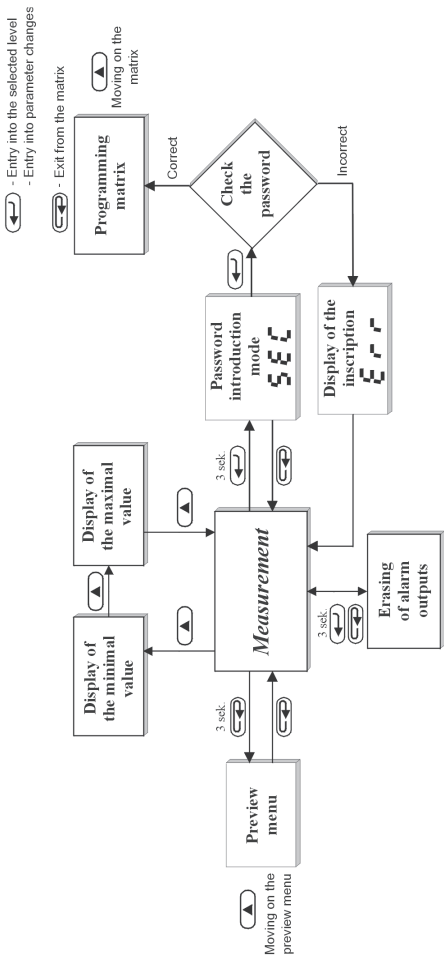





Fig 5. Servicing algorithm of the NA3 meter.

Item	Main menu	Parameters of the selected level									
		tYP	Func	Con	d_P	Cnt	i_nDI	i_H I	d_y I	i_H2	d_y2
1	Chn	Input type	Math. functions	Kind of compens.	Decim. points	Measur. time	Input individ. charact.	Param. of ind. charact.	Param. of ind. charact.	Param. of ind. charact.	
2	bAr	Bargraph type	Bargraph colour	Lower bargraph	Upper bargraph						
3	AL1	Lower threshold	Upper threshold	Alarm type	Alarm delay	Alarm support	Lower colour	Upper colour			
4	AL2	Lower threshold	Upper threshold	Alarm type	Alarm delay	Alarm support	Lower colour	Upper colour			
5	AL3	Lower threshold	Upper threshold	Alarm type	Alarm delay	Alarm support	Lower colour	Upper colour			
6	Out	Output indiv. charact.	Param. of indiv. charac.	Param. of indiv. charac.	Param. of indiv. charac.	Param. of indiv. charac.	Lower colour	Upper colour		Adr Device address	
7	SEr	Inscrip. of state param.	Password change	Test of display + bargr.	Time change	Erasing of min. value	Baud rate	Kind of transm.			
8	LOGr	Recording	Start of recording	Record date.	Record interval.						

Fig. 6. Transition matrix into the programming mode



In the table 1 programmable meter parameters are presented. The programming of parameters is possible after the previous introduction of the password.

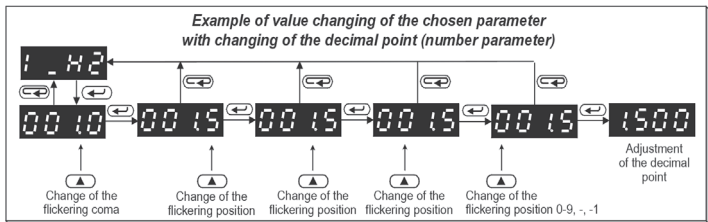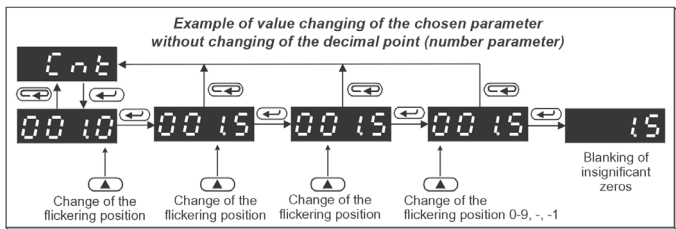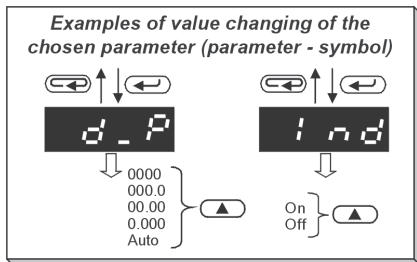



**Fig. 7.**

	Symbol on the display	Parameter description	Range of changes
Input parameter <b>Chan</b>	<b>tyP</b>	Kind of input	<p><b>Reesistance thermometers:</b>  <i>Pt 1</i> - Pt100  <i>Pt 5</i> - Pt500  <i>Pt 10</i> - Pt1000</p> <p><b>Thermocouples:</b>  <i>tE - j</i> - thermocouple, type J  <i>tE - h</i> - thermocouple, type K  <i>tE - n</i> - thermocouple, type N  <i>tE - E</i> - thermocouple, type E  <i>tE - r</i> - thermocouple, type R  <i>tE - S</i> - thermocouple, type S  <i>tE - t</i> - thermocouple, type T  <i>rE2L</i> - resistance to 400 Ω  <i>rE2H</i> - resistance to 4 kΩ  <i>nRP</i> - voltage from shunt:                      0... 60 mV</p> <p><b>Standart signals:</b>  <i>3U</i> - voltage up to 3 V  <i>10U</i> - voltage up to 10 V  <i>nARL</i> - current up to 5 mA  <i>nARH</i> - current up to 20 mA</p> <p><b>High signals:</b>  <i>200U</i> - voltage up to 200 V  <i>600U</i> - voltage up to 600 V  <i>2A</i> - current up to 2 A  <i>5A</i> - current up to 5 A</p>
	<b>Func</b>	Mathematical functions made in the channel	<p><i>OFF</i> - mathematical functions switched off;</p> <p><i>SQR</i> - raising to a power (result)<sup>2</sup></p> <p><i>SQRt</i> - extraction of roots <math>\sqrt{\text{result}}</math></p>






Input parameter <b>Chr</b>	<b>Con</b>	<p><b>Kind of compensation</b> of sensor working conditions changes:</p> <ul style="list-style-type: none"> <li>- In case of a resistance thermometer and resistance measurement it concerns the compensation of the resistance changes of the conductor linking the sensor with the meter,</li> <li>- In case of a thermocouple it concerns the compensation of reference junction temperature changes.</li> </ul> <p>The automatic compensation does not operate in case of a resistance measurement up to <b>4 kΩ</b>, <b>Pt1000</b> and <b>Pt100</b></p>	<p><b>Auto</b> - automatic compensation (in case of resistance thermometers and resistance measurement it requires a 3-wire line.)</p> <p><b>0.0...60.0°C</b> - value of the reference temperature for thermocouples.</p> <p><b>0.0...40.0 Ω</b> - resistance of two conductors for resistance thermometers and resistance measurement.</p> <p>The writing of a value beyond the interval of manual compensation will cause the <b>automatic compensation</b> switching</p>
	<b>d.p</b>	<p><b>Setting of the decimal point.</b> The setting operates both when the individual characteristic is switched off and on. The introduction of the decimal point making impossible the display of four characters on the display will cause the display of the lower or upper exceeding.</p>	<p>Setting possibility:</p> <p><b>0000</b>  <b>000.0</b>  <b>00.00</b>  <b>0.000</b></p> <p><b>Auto</b> - automatic choice of the decimal point</p>
	<b>Cnt</b>	<p><b>Averaging time of the measurement.</b></p>	<p><b>0,0...999,9 s</b></p> <p>The writing of 0 causes the switching of the measurement off and the stoppage of the meter operation. In this state, the meter displays the hour. The bargraph is blank.</p>
	<b>Indi</b>	<p>The switching off or on of the individual linear user's characteristic. - („individual characteristic of the display”).</p>	<p><b>On</b> - characteristic switched on,  <b>OFF</b> - characteristic switched off.</p> <p>When the characteristic is switched off, the meter operates with the maximal range depending on the kind of input.</p>
	<p><b>1.H1</b>  <b>d.Y1</b>  <b>1.H2</b>  <b>d.Y2</b></p>	<p><b>Parameters of the display individual characteristic.</b></p> <p>On the base of given by the user coordinates of two points the meter determines (from the system of equations) a and b coefficients of the individual characteristic.</p> $\begin{cases} d\_Y1 = a \cdot I\_H1 + b \\ d\_Y2 = a \cdot I\_H2 + b \end{cases}$ <p>Where:  I_H1 i I_H2 - measured value  d_Y1 i d_Y2 - expected value on the display.</p> <p>Fig.9 shows the way of the individual</p>	<p>Setting possibility: -1999...9999</p>

Bargraph Parameters <b>bAr</b>	<b>tyPb</b>	Bargraph type	<b>OnEc</b> - „one colour „ bargraph, : <b>ntc</b> - „ interval „ bargraph, <b>SEct</b> - „ sector“ bargraph, <b>P:nt</b> - „ point bargraph, <b>trEn</b> -"trend" bargraph. Fig. 10 explains bargraph types. .
	<b>colr</b>	Bargraph colour	<b>OFF</b> - bargraph switched off, <b>r</b> - red, <b>G</b> - green, <b>rG</b> - red + green other colours are accessible only in meters with a 7-colour bargraph. <b>b</b> - blue, <b>rb</b> - red + blue, <b>Gb</b> - green + blue, <b>rGb</b> - red + green + blue.
	<b>brL</b>	<b>Parameter to set the „magnifier” on the bargraph. Lower threshold.</b> The value of the input signal at which the bargraph is to be blank.	- 1999... 9999
	<b>brH</b>	<b>Parameter to set the „magnifier” on the bargraph. Upper threshold.</b> The value of the input signal at which the bargraph is to be lighted.	- 1999... 9999


Parameters of alarm1, alarm2 and alarm 3	<b>Prl</b>	Lower alarm threshold	- 1999... 9999
	<b>PrH</b>	Upper alarm threshold	- 1999... 9999
	<b>tyPA</b>	Alarm type Fig. 8 shows alarm types	<b>nor</b> - normal, <b>On</b> - switched on, <b>OFF</b> - switched off, <b>H_On</b> - manually switched on. Till the time of the alarm type change, the alarm output is being permanently switched on.

Parameters of alarm1, alarm2 and alarm 3			<b>H.OF</b> - manually switched off. Till the time of the alarm type change, the alarm output is being permanently switched off.
	<b>dl4</b>	<p><b>Delay of the alarm operation.</b> The parameter is defined in seconds, i.e. one must give the time in seconds after which the alarm will operate after its occurrence.</p> <p>The alarm operation follows after the measurement averaging.</p> <p>The alarm switching off follows without delay..</p>	<p><b>0.0... 999.9</b></p> <p>Introduction of <b>0.0</b> causes the operation at the moment of the alarm occurrence.</p>
	<b>HOLD</b>	<p><b>Support of alarm signalling.</b> In the situation when the holding function is switched on, after the alarm state stoppage, the alarm is still switched on (alarm diode, relay or OC contacts).</p> <p>The alarm state is active till the moment of erasing it by means of the combination of  and  keys. Hold down within ca 3 seconds.</p>	<p><b>OFF</b> - The maintenance of the alarm output is switched off.</p> <p><b>On</b> - The maintenance of the alarm output is switched on.</p>
	<b>Curl</b>	<b>Colour of the lower threshold alarm marker.</b>	<b>OFF</b> - alarm marker switched off.
	<b>CurH</b>	<b>Colour of the upper threshold alarm marker.</b>	<p><b>r</b> - red,</p> <p><b>G</b> - green,</p> <p><b>rG</b> - red + green,</p> <p>Other colours are accessible only in meters with a 7-colour bargraph.</p> <p><b>b</b> - blue,</p> <p><b>rb</b> - red + blue,</p> <p><b>Gb</b> - green + blue,</p> <p><b>rGb</b> - red + green + blue,</p> <p>Fig. 10 explains the idea of Curl and CurH... parameters</p>

Output parameters	<b>:nd0</b>	Switching off or on of the individual linear user's characteristic - („ <b>individual characteristic of the analog output</b> “).	<b>0n</b> - characteristic switched on, <b>OFF</b> - characteristic switched off . When the characteristic is switched off, the meter operates at the maximal range depending on input and range output.
	<b>d-H1</b> <b>O-Y1</b> <b>d-H2</b> <b>O-Y2</b>	<b>Parameters of the individual characteristic of the analog output.</b> On the base of given coordinates of two points by the user, the meter determines (from the equation system) coefficients a and b of the individual characteristic. $\begin{cases} O\_Y1 = a \cdot d\_H1 + b \\ O\_Y2 = a \cdot d\_H2 + b \end{cases}$ where: d_H1 and d_H2 - displayed value O_Y1 and O_Y2 - expected value on the analog output. Fig. 9 represents the graphical illustration explaining the idea of the individual characteristic.	Setting possibility: - <b>1999... 9999</b>
	<b>bAud</b>	<b>Baud rate of the RS-485 interface.</b>	<b>2400</b> - 2400 b/s <b>4800</b> - 4800 b/s <b>9600</b> - 9600 b/s
	<b>trYb</b>	<b>Kind of transmission through the RS-485 interface.</b>	<b>OFF</b> - interface switched off <b>8n1</b> - ASCII 8N1 <b>7E1</b> - ASCII 7E1 <b>7O1</b> - ASCII 7O1 <b>r8n2</b> - RTU 8N2 <b>r8E1</b> - RTU 8E1 <b>r8o1</b> - RTU 8O1 <b>r8n1</b> - RTU 8N1
	<b>Adr</b>	<b>Device address</b>	0...247


Servicing parameters SEr	SEt	<b>Manufacturer's parameters.</b> Manufacturer's parameters are presented in the table 2.	The pressure of the  key causes the writing of manufacturer's parameters.
	SEc	<b>Introduction of a new password.</b>	- 1999... 9999
	tSt	<b>Test of displays.</b> The test consists on a successive display of numbers 1111, 2222 etc. Successive bargraph colours are lighted on the bargraph.	The pressure of the  key causes the test switching on. The pressure of the  key ends the test.
	Hour	<b>Setting of the current time.</b> Time format : hh:mm:ss	00:00:00 ... 23:59:59
	CLrL	<b>Erasing of the minimal value.</b>	The pressure of the  key causes the erasing of the minimal value.
CLrH	<b>Erasing of the maximal value.</b>	The pressure of the  key causes the erasing of the maximal value.	

Recording parameters LOEr	rEE	<b>Switching the recording on or off.</b> At the moment of switching the recording on, the meter erases the previous stored values.	On - recording switched on OFF - recording switched off
	Lo-r	<b>Hour of recording start</b> Time format: hh:mm:ss	00:00:00 ... 23:59:59
	dAtE	<b>Date of recording start</b> Date format: yy.mm.dd It is an information parameter. It not serves to define the date from which the recording is to begin, but only to inform when the recording	70.01.01 ... 38.12.31
	intE	<b>Time interval of recording -</b> Defines the segment of time and at which sequence the result will be to memorised. Minimal interval 1 s. Format: hh:mm:ss	00:00:00 ... 99:59:59

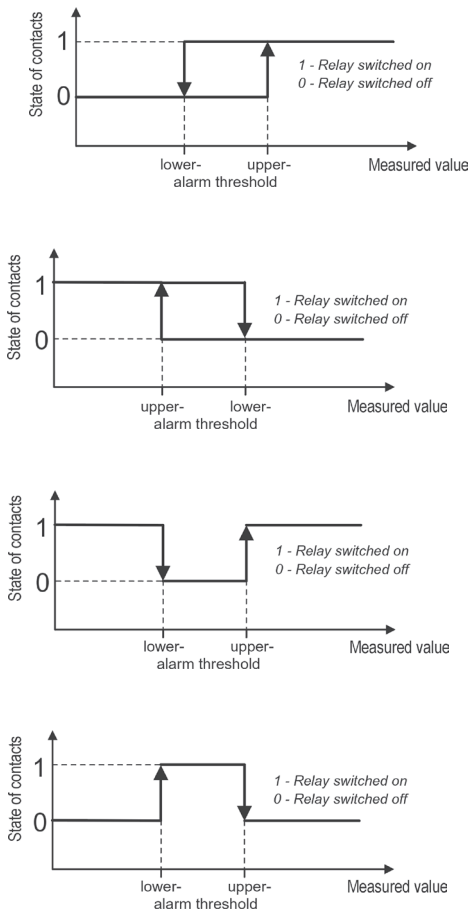


**Fig. 8. Alarm types: a, b - normal, c - switched off, d - switched on**



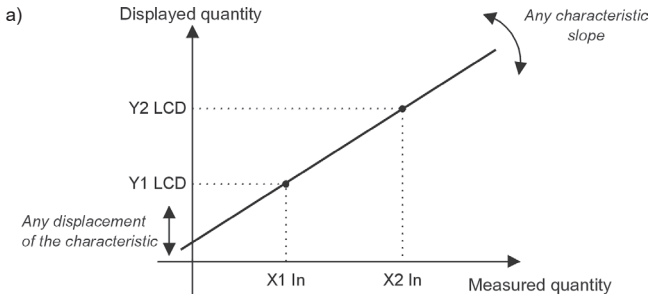

Value  $I_{H1}$  on the meter input  $\Rightarrow$   $d_{Y1}$  on the display.  
 Value  $I_{H2}$  on the meter input  $\Rightarrow$   $d_{Y2}$  on the display  
 other points of the characteristic are evaluated

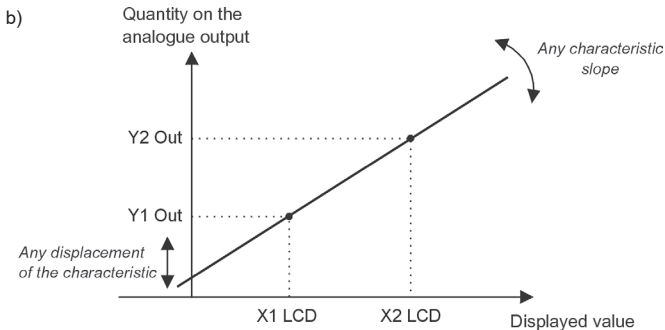

Value  $d_{H1}$  on the display  $\Rightarrow$   $0_{Y1}$  on the analogue output.  
 Value  $I_{H2}$  on the display  $\Rightarrow$   $d_{Y2}$  on the analogue output  
 other points of the characteristic are evaluated

**Fig. 9. Individual characteristic of the display a) and analogue output b).**

Type of bargraph	Exemplary settings of the bargraph and the alarm, ex. 1 $CurL = G$ (green) $CurL = r$ (red) $CurH = rG$ (red + green)	Notes
<i>OnEL</i>		
<i>:nt r</i>		Value under the value $P_{rL}$
		Value between $P_{rL}$ and $P_{rH}$
		Value over $P_{rH}$
<i>SEct</i>		
<i>P:nt</i>		
<i>trEn</i>		Value without changes in time
		Value increases
		Value decreases

**Fig. 10. Bargraph modes.**



**NOTE!**

- In case of the meter working with a resistance thermometer in a two-wire system, the choice of the automatic compensation of conductor resistance changes will cause a meter defective work.
- The automatic compensation is switched off when choosing Pt1000, Pt500 sensors and at measuring the resistance up to 4 k $\Omega$ . Connect the signal only in the two-wire system.
- In case of switching the display individual characteristic on, the result on the display is lineally converted in accordance with the introduced  $I_{H1}$ ,  $I_{H2}$ ,  $d_{Y1}$  and  $d_{Y2}$  parameters.
- In case of switching the analogue output individual characteristic on, the measurement result is lineally converted in accordance with the introduced  $d_{H1}$ ,  $d_{H2}$ ,  $O_{Y1}$  and  $O_{Y2}$  parameters.

- The meter checks currently the value of the introduced parameter. In case when the introduced value exceeds the upper or lower change range given in the table 1, the meter will not make the parameter record.
- In case of the **Input type** change, a simultaneous change of the decimal point follows, optimally for the given input.
- After the supply decay, the current time is reset.
- The switching of the record off follows in following cases: switching the record off from the programming matrix, change of the input kind, change of Go\_r, change of IntE, setting Cnt=0, memory filling up and when the meter is switched to the network on again.
- In case of the Intr or Sect bargraph type, the setting of Curl and Curh markers (from one alarm) is possible. The others are automatically erased.
- Max. and min. values are erased in case of following changes: input type, individual characteristic (on, off), entry of standard parameters.

Standard parameters of the NA3 meter

Table 2

Parameter description	Standard value	Parameter description	Standard value
<i>tYP</i>	Pt100	<i>MOld</i>	OFF
<i>Func</i>	OFF	<i>Curl</i>	r
<i>Con</i>	0 = manual	<i>Curh</i>	rG
<i>d.P</i>	0000.0	<i>:nd0</i>	OFF
<i>Cnt</i>	1.0	<i>d.H1</i>	0
<i>:nd1</i>	OFF	<i>D.Y1</i>	
<i>:.H1</i>	0	<i>d.H2</i>	
<i>d.Y1</i>		<i>D.Y2</i>	
<i>:.H2</i>		<i>bAud</i>	9600
<i>d.Y2</i>		<i>trYb</i>	RTU 8N2
<i>tYPb</i>	Sect	<i>Rdr</i>	1
<i>colr</i>	G	<i>SEC</i>	0
<i>brL</i>	- 200	<i>Hour</i>	00:00:00
<i>brH</i>	850	<i>rEC</i>	OFF
<i>PrL</i>	- 200	<i>Go_r</i>	00:00:00
<i>PrH</i>	850.0	<i>dAtE</i>	70.01.01
<i>tYPR</i>	OFF	<i>:ntE</i>	00:15:00
<i>dLY</i>	0		

## 6. RS-485 INTERFACE

NA3 programmable digital meters have a serial link of RS-485 standard to communicate in computer systems and with other devices fulfilling the master function. The MODBUS asynchronous character communication protocol has been implemented on the serial link. The transmission protocol describes information exchange procedures between devices through the serial link.

### 6.1. Procedure of the serial interface connection

The RS-485 standard enables the direct connection to 32 devices on a single serial link up to a 1200 m distance. For the connection of a higher number of devices it is necessary to apply additional intermediate-to-separating systems.

The exit of the interface line is presented in the service manual on the fig. 3.d. In order to obtain a correct transmission it is necessary to connect lines **A** and **B** in parallel to their equivalent lines in other devices.

The connection must be made with a shielded conductor. The shield must be connected to the protective terminal in one point.

The **GND** line serves to the additional protection of the interface line at long distance connections.

One must connect GND signals between devices and one point to the protective terminal (that is not necessary for the interface correct operation).

To obtain the connection with the computer of IBM PC class, an RS-232 into RS-485 converter of PD5 type is necessary or an RS-485 interface card. The way of NA3 meter connection through the PD5 converter is shown on the fig. 3d.

The designation of transmission lines for the card in the PC computer depends on the card producer.

### 6.2. Description of the MODBUS protocol implementation

The implemented protocol is in accordance with the PI-MBUS-300 Rev G Modicon company specification.

The set of parameters of the meter serial link in the MODBUS protocol:

- |                         |   |
|-------------------------|---|
| – meter address         | 1... 247  |
| – baud rate             | 2400, 4800, 9600 bit/s                          |
| – working mode          | ASCII, RTU                                      |
| – information unit      | ASCII: 8N1, 7E1, 7O1<br>RTU: 8N2, 8N1, 8E1, 8O1 |
| – maximal response time | 300 ms  |

The configuration of serial link parameters is described in the further part of this service manual. It consists on the settlement of the baud rate (**Baud** parameter), device address (**Adr** parameter), and the type of the information unit (**Tryb** parameter)

**Note:** Each meter connected to the communication network must:

- have a unique address, different from addresses of other devices connected to the network
- the identical baud rate and the type of the information unit.

### 6.3 Description of the MODBUS protocol function

Following functions of the MODBUS protocol have been implemented in NA3 meters:

#### Bit-8 Error of the conductor resistance compensation

Function description

Table 3

<i>Code</i>	<i>Meaning</i>
03 (03 h)	Read-out of n-registers
06 (06 h)	Recording of a single register
16 (10 h)	Recording of n-registers
17 (11 h)	Identification of the slave device

**Note:**

In NA3 meters the answer response frame to the function 17 is as follows:

Device address	Function	Number of bytes	Device identifier	Device state	Field depending on the type of device	Check-sum
X	11	08	X	FF	XXXXXX	

#### Read-out of n-registers (code 03 h)

The function is inaccessible in the publication mode.

**Example:** read-out of 2 registers starting from the register which the address is 1 DBDh (7613) in RTU mode.

Request:

Device address	Function	Register address Hi	Register address Lo	Number of registers Hi	Number of registers Lo	Check-sum CRC
01	03	1D	BD	00	02	52 43

Response:

Device address	Function	Number of bytes	Value from the register 1DBD (7613)				Value from the register 1DBE (7614)				Check-sum CRC
			3F	80	00	00	40	00	00	00	
01	03	08	3F	80	00	00	40	00	00	00	42 8B

### Recording of values into the register (code 06h)

The function is accessible in the publication mode.

**Example:** recording of the register which address is 1DBDh (7613) in RTU mode.

Request:

Device address	Function	Register address Hi	Register address Lo	Value from the register 1DBD (7613)				Check-sum CRC
				3F	80	00	00	
01	06	1D	BD	3F	80	00	00	85 AD

Response:

Device address	Function	Register address Hi	Register address Lo	Value from the register 1DBD (7613)				Check-sum CRC
				3F	80	00	00	
01	06	1D	BD	3F	80	00	00	85 AD

### Recording into n-registers (code 10h)

The function is accessible in the publication mode

**Example:** recording of 2 registers starting from the register which address is 1DBDh (7613) in RTU mode.

Request:

Device address	Function	Register address		Number of registers		Number of bytes	Value for the register 1DBD (7613)				Value for the register 1DBE (7614)				Check-sum CRC
		Hi	Lo	Hi	Lo		3F	80	00	00	40	00	00	00	
01	10	1D	BD	00	02	08	3F	80	00	00	40	00	00	00	03 09

Response:

Device address	Function	Register address Hi	Register address Lo	Number of registers Hi	Number of registers Lo	Check-sum (CRC)

## Report identifying devices (code 11h) in RTU mode.

**Example:** the read-out of data identifying the device for NA3 meter with a universal input

Request:

Device address	Function	Checksum (CRC)
01	11	C0 2C

Response:

Device address	Function	Number of bytes	Device identifier	Device state	Field depending on the type of device	Checksum
01	11	08	80	FF	00XXXXX	

**Device address** - depending on the set point

**Function** - no of function 0 x 11

**Number of bytes** - 0x08

**Device identifier**

- 0x80 - NA3 with universal input (NA3-XXXU)
- 0x85 - NA3 with temperature input (NA3-XXXT)
- 0x86 - NA3 with standard input (NA3-XXXS)
- 0x87 - NA3 with high signal input (NA3-XXXH)

**Device state** - 0xFF

**Field depending on the device type** - XXXXXX

Device name - transmitted as ASCII character and defines the meter type:

U - 0x55, 55 X X X X X

T - 0x54, 54 X X X X X

S - 0x53, 53 X X X X X

H - 0x48, 48 X X X X X

Analogue output

- field depending on the type of the analogue output
- 0x00 - lack of analogue output, X 00 X X X X
- 0x01 - voltage analogue output, X 01 X X X X
- 0x02 - current analogue output, X 02 X X X X

No. of the software  
version

- software version implemented in the meter
- X X \_ \_ \_ 4 - byte variable of float type

**Checksum**

- 2 bytes in case of work in RTU mode
- 1 byte in case of work in ASCII mode

**Example:**

Work in **RTU** mode, e.g.: **Mode = RTU 8N2** (value 0x02 in case of readout/record through the interface).

**NA3** meter with an universal input (NA3-XXXU)

Execution with a voltage analogue output: **00**,

No. of the software version: **1.00**,

Device address set on: **Adr = 0 x 01**,

For such a meter the frame has the following form:

Device address	Function	Number of bytes	Device identifier	Device state	Field depending on the device type	Check-sum (CRC)
01	11	08	80	FF	00 00 3F 80 00 00	3F 1B

## 6.4. Register map of NA3 meters

Register map of NA3 meters

Table 4.

<b>Address range</b>	<b>Type of value</b>	<b>Description</b>
7000-7200	Float (32 bits)	The value is placed in two successive 16-bytes registers. Registers enclose the same data as 32-bytes registers from the 7500 area. Registers are only for readout.
7200-7400	Float (32 bits)	The value is placed in two successive 16-bit registers. Registers enclose the same data as 32-bit registers from the 7600 area. Registers can be readout and written.
7500-7600	Float (32 bits)	The value is placed in a 32-bytes register. Registers are only for readout.
7600-7700	Float (32 bits)	The value is placed in a 32-bit register. Registers can be read out and written.



## 6.5. Registers for recording and readout

### NA3 meter

The value is placed in two successive 16-bit registers enclosing the same data as 32-bit registers from the 7600 area	The value is placed in 32-bit registers	Symbol	Writing (w) Readout (r)	Range	Description																																												
7200	7600	<b>Identifier</b>	r	-	Device identifier																																												
					<table border="1"> <thead> <tr> <th data-bbox="606 480 678 509">Value</th> <th data-bbox="688 480 947 509"></th> </tr> </thead> <tbody> <tr> <td data-bbox="606 516 678 546">80</td> <td data-bbox="688 516 947 546">NA3 with universal input „U”</td> </tr> <tr> <td data-bbox="606 546 678 575">85</td> <td data-bbox="688 546 947 575">NA3 with temperature input „T”</td> </tr> <tr> <td data-bbox="606 575 678 604">86</td> <td data-bbox="688 575 947 604">NA3 with standard input „S”</td> </tr> <tr> <td data-bbox="606 604 678 618">87</td> <td data-bbox="688 604 947 618">NA3 with high signal input „H”</td> </tr> </tbody> </table>	Value		80	NA3 with universal input „U”	85	NA3 with temperature input „T”	86	NA3 with standard input „S”	87	NA3 with high signal input „H”																																		
Value																																																	
80	NA3 with universal input „U”																																																
85	NA3 with temperature input „T”																																																
86	NA3 with standard input „S”																																																
87	NA3 with high signal input „H”																																																
7202	7601	<b>Channel number</b>	w/r	0...1	No occurs																																												
7204	7602	<b>Output type</b>	w/r	0...20	Input type																																												
					<table border="1"> <thead> <tr> <th data-bbox="606 720 678 749">Value</th> <th data-bbox="688 720 947 749"></th> </tr> </thead> <tbody> <tr><td data-bbox="606 757 678 778">0</td><td data-bbox="688 757 947 778">Pt100 RTD</td></tr> <tr><td data-bbox="606 778 678 800">1</td><td data-bbox="688 778 947 800">Pt500 RTD</td></tr> <tr><td data-bbox="606 800 678 822">2</td><td data-bbox="688 800 947 822">Pt1000 RTD</td></tr> <tr><td data-bbox="606 822 678 844">3</td><td data-bbox="688 822 947 844">J thermocouple</td></tr> <tr><td data-bbox="606 844 678 866">4</td><td data-bbox="688 844 947 866">K thermocouple</td></tr> <tr><td data-bbox="606 866 678 888">5</td><td data-bbox="688 866 947 888">N thermocouple</td></tr> <tr><td data-bbox="606 888 678 910">6</td><td data-bbox="688 888 947 910">E thermocouple</td></tr> <tr><td data-bbox="606 910 678 931">7</td><td data-bbox="688 910 947 931">R thermocouple</td></tr> <tr><td data-bbox="606 931 678 953">8</td><td data-bbox="688 931 947 953">S thermocouple</td></tr> <tr><td data-bbox="606 953 678 975">9</td><td data-bbox="688 953 947 975">T thermocouple</td></tr> <tr><td data-bbox="606 975 678 997">10</td><td data-bbox="688 975 947 997">R. meas. up to 400 Ω</td></tr> <tr><td data-bbox="606 997 678 1019">11</td><td data-bbox="688 997 947 1019">R. meas. up to 4 kΩ</td></tr> <tr><td data-bbox="606 1019 678 1041">12</td><td data-bbox="688 1019 947 1041">Volt. meas. 0... 60 mV</td></tr> <tr><td data-bbox="606 1041 678 1062">13</td><td data-bbox="688 1041 947 1062">Volt. meas. 0... 3 V</td></tr> <tr><td data-bbox="606 1062 678 1084">14</td><td data-bbox="688 1062 947 1084">Volt. meas. 0...10 V</td></tr> <tr><td data-bbox="606 1084 678 1106">15</td><td data-bbox="688 1084 947 1106">Current meas. 0... 5 mA</td></tr> <tr><td data-bbox="606 1106 678 1128">16</td><td data-bbox="688 1106 947 1128">Current meas. 0... 20 mA</td></tr> <tr><td data-bbox="606 1128 678 1150">17</td><td data-bbox="688 1128 947 1150">Volt. meas. 0... 200 V</td></tr> <tr><td data-bbox="606 1150 678 1172">18</td><td data-bbox="688 1150 947 1172">Volt. meas. 0... 600 V</td></tr> <tr><td data-bbox="606 1172 678 1193">19</td><td data-bbox="688 1172 947 1193">Current meas. 0...2 A</td></tr> <tr><td data-bbox="606 1193 678 1215">20</td><td data-bbox="688 1193 947 1215">Current meas. 0...5 A</td></tr> </tbody> </table>	Value		0	Pt100 RTD	1	Pt500 RTD	2	Pt1000 RTD	3	J thermocouple	4	K thermocouple	5	N thermocouple	6	E thermocouple	7	R thermocouple	8	S thermocouple	9	T thermocouple	10	R. meas. up to 400 Ω	11	R. meas. up to 4 kΩ	12	Volt. meas. 0... 60 mV	13	Volt. meas. 0... 3 V	14	Volt. meas. 0...10 V	15	Current meas. 0... 5 mA	16	Current meas. 0... 20 mA	17	Volt. meas. 0... 200 V	18	Volt. meas. 0... 600 V	19	Current meas. 0...2 A	20	Current meas. 0...5 A
Value																																																	
0	Pt100 RTD																																																
1	Pt500 RTD																																																
2	Pt1000 RTD																																																
3	J thermocouple																																																
4	K thermocouple																																																
5	N thermocouple																																																
6	E thermocouple																																																
7	R thermocouple																																																
8	S thermocouple																																																
9	T thermocouple																																																
10	R. meas. up to 400 Ω																																																
11	R. meas. up to 4 kΩ																																																
12	Volt. meas. 0... 60 mV																																																
13	Volt. meas. 0... 3 V																																																
14	Volt. meas. 0...10 V																																																
15	Current meas. 0... 5 mA																																																
16	Current meas. 0... 20 mA																																																
17	Volt. meas. 0... 200 V																																																
18	Volt. meas. 0... 600 V																																																
19	Current meas. 0...2 A																																																
20	Current meas. 0...5 A																																																

7206	7603	<b>L0In</b>	w/r	-1999... 9999	No occurs	
7208	7604	<b>Hiln</b>	w/r	-1999... 9999	No occurs	
7210	7605	<b>Function</b>	w/r	0... 2	Arithmetical function	
					<b>Value</b>	
					0	Switched off
					1	Squaring
					2	Extraction of roots
7212	7606	<b>Compens.</b>	w/r	-199.9... 999.9	Compensation of the conductor resistance	
7214	7607	<b>D_P</b>	w/r	0... 4	Decimal point	
					<b>Value</b>	
					0	0000
					1	000.0
					2	00.00
					3	0.000
					4	Auto
7216	7608	<b>Cnt</b>	w/r	0... 999.9	Measurement time	
7218	7609	<b>Indi</b>	w/r	0... 1	Individual characteristic	
					<b>Value</b>	
					0	Switched characteristic off
					1	Switched characteristic on
7220	7610	<b>X1 In</b>	w/r	-1999... 9999	Parameters of the individual characteristic	
7222	7611	<b>Y1 LED</b>	w/r	-1999... 9999	Parameters of the individual characteristic	
7224	7612	<b>X2 In</b>	w/r	-1999... 9999	Parameters of the individual characteristic	
7226	7613	<b>Y2 LED</b>	w/r	-1999... 9999	Parameters of the individual characteristic	
7228	7614	<b>Bargraph number</b>	w/r	0... 1	No occurs	
7230	7615	<b>Bargraph type</b>	w/r	0... 4	Bargraph type	
					<b>Value</b>	
					0	One-colour ( <b>OnEC</b> )
					1	Change of colour after exceeding the alarm threshold (the colour change the whole bargraph) ( <b>Intr</b> )

					2	Change of colour after exceeding the alarm threshold (Three-segment change of colour) ( <b>SEct</b> )
					3	One-coloured bargraph, alarm markers in another colour ( <b>PInt</b> )
					4	Increasing/decreasing trend ( <b>trEn</b> )
7232	7616	<b>Colour</b>	w/r	0... 7	Bargraph colour	
					<b>Value</b>	
					0	Bargraph off ( <b>OFF</b> )
					1	Red ( <b>r</b> )
					2	Green ( <b>G</b> )
					3	Red + Green ( <b>rG</b> )
					Other values are only accessible in meters with RGB diodes	
					4	Blue ( <b>b</b> )
					5	Red + Blue ( <b>rb</b> )
					6	Green + blue ( <b>Gb</b> )
					7	Red + Green + Blue ( <b>rGb</b> )
7234	7617	<b>Brl</b>	w/r	-1999... 9999	„Magnifier „on the bargraph. Lower threshold	
7236	7618	<b>Brh</b>	w/r	-1999... 9999	„Magnifier „on the bargraph. Upper threshold	
7238	7619	<b>Alarm number</b>	w/r	0... 2	Choice of alarm number	
					Range of changes is depended on the meter execution code (number of alarms)	
7240	7620	<b>Ch_Alarm</b>	w/r	0... 1	No occurs	
7242	7621	<b>Pri</b>	w/r	-1999... 9999	Alarm lower threshold < <b>Alarm No</b> >	
7244	7622	<b>Prh</b>	w/r	-1999... 9999	Alarm upper threshold < <b>Alarm No</b> >	
7246	7623	<b>Type a</b>	w/r	0... 4	Alarm type < <b>Alarm No</b> >	
					<b>Value</b>	
					0	Normal
					1	Switched on
					2	Switched off
					3	Manually switched on
					4	Manually switched off

7248	7624	<b>Alarm delay</b>	w/r	0... 999.9	Alarm delay <Alarm No>	
7250	7625	<b>Alarm support</b>	w/r	0... 1	Alarm signalling support <Alarm No>	
					<b>Value</b>	
					0	Support switched off
					1	Support switched on
7252	7626	<b>CURL</b>	w/r	0... 7	Bargraph colour for the lower alarm threshold	
					<b>Value</b>	
					0	Bargraph switched off ( <b>OFF</b> )
					1	Red ( <b>r</b> )
					2	Green ( <b>G</b> )
					3	Red + Green ( <b>rG</b> )
					Other values accessible only in meters with RGB diodes	
					4	Blue ( <b>b</b> )
					5	Red + Blue ( <b>rb</b> )
					6	Green + blue ( <b>Gb</b> )
					7	Red + Green + Blue ( <b>rGb</b> )
7254	7627	<b>CURH</b>	w/r	0... 7	Bargraph colour after exceeding the upper alarm threshold <Alarm No>	
					<b>Value</b>	
					0	Bargraph switched off ( <b>OFF</b> )
					1	Red ( <b>r</b> )
					2	Green ( <b>G</b> )
					3	Red + Green ( <b>rG</b> )
					Other values accessible only in meters with RGB diodes	
					4	Blue ( <b>b</b> )
					5	Red + Blue ( <b>rb</b> )
					6	Green + blue ( <b>Gb</b> )
					7	Red + Green + Blue ( <b>rGb</b> )
7256	7628	<b>Chna</b>	w/r	0... 1	No occurs	
7258	7629	<b>Output characteristic</b>	w/r	0... 1	Characteristic of the analogue output	
					<b>Value</b>	
					0	Characteristic switched off
					1	Characteristic switched on

7260	7630	<b>X1 LED</b>	w/r	- 1999... 9999	Parameters of the analogue output characteristic	
7262	7631	<b>Y1 Out</b>	w/r	- 1999... 9999	Parameters of the analogue output characteristic	
7264	7632	<b>X2 LED</b>	w/r	- 1999... 9999	Parameters of the analogue output characteristic	
7266	7633	<b>Y2 Out</b>	w/r	- 1999... 9999	Parameters of the analogue output characteristic	
7268	7634	<b>Baud rate</b>	w/r	0... 2	Baud rate of the RS-485 interface	
					<b>Value</b>	
					0	2400 bit/s
					1	4800 bit/s
					2	9600 bit/s
7270	7635	<b>Working mode</b>	w/r	1... 7	Working mode of the MODBUS protocol	
					<b>Value</b>	
					1	ASCII 8N1
					2	ASCII 7E1
					3	ASCII 7O1
					4	RTU 8N2
					5	RTU 8E2
					6	RTU 8O2
					7	RTU 8N1
7272	7636	<b>Address</b>	w/r	0... 247	Choice of the device address	
7274	7637	<b>Test</b>	w/r	0... 1	Test of the display	
					<b>Value</b>	
					0	Lack of operation
					1	Test
7276	7638	<b>Hour</b>	w/r	0... 23.5959	Current time	
					<p>This parameter occurs with four places after the decimal point in format gg,mmss, where:</p> <p>gg - means hours,  mm - means minutes,  ss - means seconds</p> <p>In case when introducing and incorrect time, the indicator will correct it automatically.</p>	
7278	7639	<b>Recording</b>	w/r	0... 1	Registration of measured value	
					<b>Value</b>	
					0	Registration switched off
					1	Registration switched on

7280	7640	<b>Interval</b>	w/r	0... 99.5959	Time interval of the recording						
7282	7642	<b>Recording time</b>	w/r	0... 23.5959	Time of the recording start						
					<p>This parameter occurs with four places after the decimal point in format gg,mmss, where:</p> <p>gg - means hours, mm - means minutes, ss - means seconds</p> <p>In case when introducing and incorrect time, the indicator will correct it automatically.</p>						
7284	7642	<b>Year</b>	w/r	1970... 2038	Year of the recording start						
7286	7643	<b>Month</b>	w/r	1... 12	Month of the recording start						
7288	7644	<b>Day</b>	w/r	1... 31	Day of the recording start						
					<p>Year, Month, Day are information parameters. They do not serve to define the date from which the recording is to be start, but only to inform since when the recording has started.</p>						
7290	7645	<b>Erasing of minimum Channel 1</b>	w/r	0... 1	Erasing of the minimal value						
					<table border="1"> <tr> <td><b>Value</b></td> <td></td> </tr> <tr> <td>0</td> <td>Lack of operation</td> </tr> <tr> <td>1</td> <td>Erasing</td> </tr> </table>	<b>Value</b>		0	Lack of operation	1	Erasing
<b>Value</b>											
0	Lack of operation										
1	Erasing										
7292	7646	<b>Erasing of maximum Channel 1</b>	w/r	0... 1	Erasing of the maximal value						
					<table border="1"> <tr> <td><b>Value</b></td> <td></td> </tr> <tr> <td>0</td> <td>Lack of operation</td> </tr> <tr> <td>1</td> <td>Erasing</td> </tr> </table>	<b>Value</b>		0	Lack of operation	1	Erasing
<b>Value</b>											
0	Lack of operation										
1	Erasing										
7294	7647	<b>Erasing of minimum Channel 2</b>	w/r	0... 1	No occurs						
7296	7648	<b>Erasing of minimum Channel 2</b>	w/r	0... 1	No occurs						

7320	7660	<b>Year of the memorised value</b>	w/r	1970... 2038	Year of memorised value in memory
7322	7661	<b>Month of the memorised value</b>	w/r	1... 12	Month of memorised value in memory
7324	7662	<b>Day of the memorised value</b>	w/r	1... 31	Day of memorised value in memory

7326	7663	<b>Time of the memorised value</b>	w/r	0... 23.5959	Time of memorised value in memory																
					<p>This parameter occurs with four places after the decimal point in format gg.mmss, where:</p> <p>gg - means hours, mm - means minutes, ss - means seconds</p> <p>In case when introducing and incorrect time, the meter will correct it automatically.</p>																
7328	7664	<b>Index of the memorised value</b>	w/r	1... 750	Number of memorised value in memory																
7230	7665	<b>Status</b>	w/r	0... 8	Operation status on the buffer																
					<table border="1"> <thead> <tr> <th>Value</th> <th></th> </tr> </thead> <tbody> <tr> <td>0</td> <td>Lack of operation</td> </tr> <tr> <td>1</td> <td>Searching acc. date and time (registers nr 7660...7663 and 7320...7326)</td> </tr> <tr> <td>2</td> <td>Searching acc. time (registers nr 7663 and 7326)</td> </tr> <tr> <td>3</td> <td>Searching acc. index (registers nr 7664 and 7328)</td> </tr> <tr> <td>4</td> <td>Load next values into the buffer (registers7672...7691and 7344...7382)</td> </tr> <tr> <td>5</td> <td>Load previous values into the buffer (registers7672...7691 and 7344...7382)</td> </tr> <tr> <td>6</td> <td>Go to the first memorised value in memory.</td> </tr> </tbody> </table>	Value		0	Lack of operation	1	Searching acc. date and time (registers nr 7660...7663 and 7320...7326)	2	Searching acc. time (registers nr 7663 and 7326)	3	Searching acc. index (registers nr 7664 and 7328)	4	Load next values into the buffer (registers7672...7691and 7344...7382)	5	Load previous values into the buffer (registers7672...7691 and 7344...7382)	6	Go to the first memorised value in memory.
Value																					
0	Lack of operation																				
1	Searching acc. date and time (registers nr 7660...7663 and 7320...7326)																				
2	Searching acc. time (registers nr 7663 and 7326)																				
3	Searching acc. index (registers nr 7664 and 7328)																				
4	Load next values into the buffer (registers7672...7691and 7344...7382)																				
5	Load previous values into the buffer (registers7672...7691 and 7344...7382)																				
6	Go to the first memorised value in memory.																				

					7	Go to the last memorised value in memory.
					8	Erase the memory
7332	7666	<b>Number of the memorised value</b>	r	0... 750	Number of memorised value in memory, placed in the first buffer register	
					<b>Value</b>	
					0	Memory is empty
					1... 750	Number of the memorised value
7334	7667	<b>Number of recorded registers</b>	r	0... 750	Number of recorded buffer registers	
					<b>Value</b>	
					0	Buffer is empty
					1... 750	Number of recorded registers
7336	7668	<b>Year</b>	r	1970... 2038	Year for the value in the first register	
7338	7669	<b>Month</b>	r	1... 12	Month for the value in the first register	
7340	7670	<b>Day</b>	r	1... 31	Day for the value in the first register	
7342	7671	<b>Time</b>	r	0... 23.5959	Time for the value in the first register	
					This parameter occurs with four places after the decimal point in format gg.mmss, where: gg - means hours, mm - means minutes, ss - means seconds	
7344...7382	7672...7691	<b>Buffer</b>	r	-	Memorised values, read out from the memory	
					20 registers , including 20 memorised values.	

1) In case of registers not occurring in the given meter series, their value



## 6.6. Registers only for readout

### NA3 meter


The value is placed into two successive 16-bit registers. These registers include the same data as 32-bit registers from the area 7500.	The value is placed into 32-bit registers	Name	Writing (w) Readout (r)	Unit	Quantity name
7002	7501	<b>Status 1</b>	r	-	Register describing the current state of the meter
7004	7502	<b>Status 2</b>	r	-	Register describing the current state of the meter
7006	7503	<b>Steering out</b>	r	%	It is the register defining the control procedure of the analogue output (controllability)
7008	7504	<b>Min 1</b>	r	-	Minimal value of the currently measured value of channel 1
7010	7505	<b>Max 1</b>	r	-	Maximal value of the currently measured value of channel 1
7012	7506	<b>Value 1</b>	r	-	Currently measured value of channel 1
7014	7507	<b>Hour</b>	r		Current time
7016	7508	<b>Min 2</b>	r	-	No occurs
7018	7509	<b>Max 2</b>	r	-	No occurs
7020	7510	<b>Value 2</b>	r	-	No occurs

1) In case of registers no occurring in the given meter series, their values is 1E+20

#### Note !

- At the moment of exceeding the upper or lower range, „displayed value“, „minimum“, „maximum“ parameters are set on the value 1E+20.
- For the parameter **Cnt**=0 (Measurement switching off and display of the current time), „minimum“, „maximum“ and „displayed value“ parameters are set on the value 1E+20.

## Description of the Status 1 register

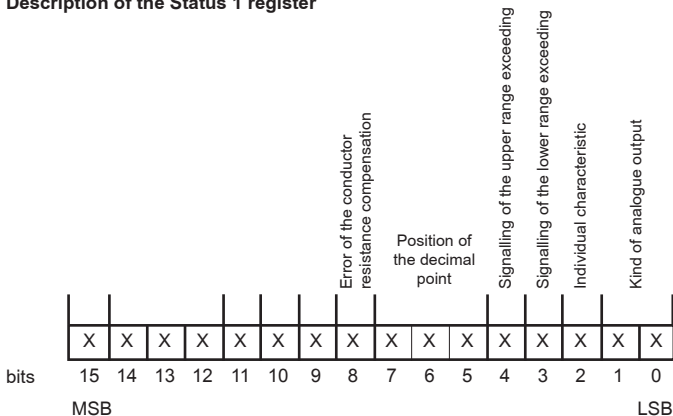

0 - Lack of error

1 - Signalling of compensation error

### Bit-7...5 Position of the decimal point

000 - lack

001 - 000.0

010 - 00.00

011 - 0.000

100 - Auto

### Bit-4 Signalling of the upper range exceeding

0 - normal work

1 - range exceeding

### Bit-3 Signalling of the lower range exceeding

0 - normal work

1 - range exceeding

### Bit-2 Individual characteristic

0 - individual characteristic switched off

1 - individual characteristic switched on

#### Bit-1...0 Kind of output (voltage, current)


00 - lack of analogue output

01 - current

10 - voltage

#### Bit-15. No used

### Description of the status 2 register

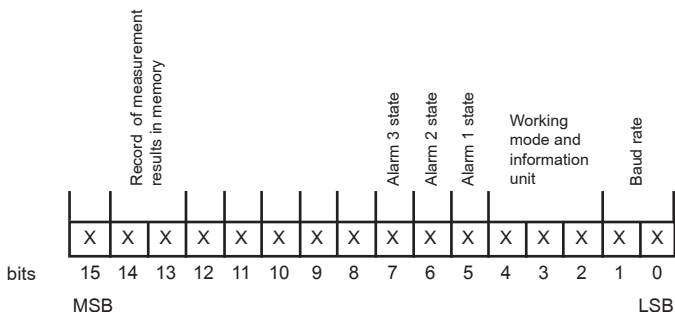

#### Bit-14...13 Record of measurement results in memory

0 - Record switched off

1 - Record switched on

#### Bit-12...8 . No used

#### Bit-7. State of alarme 3

0 - off

1 - on

#### Bit-6 State of alarm 2

0 - off

1 - on

**Bit-5 State of alarm 1**

0 - off

1 - on

**Bit-4...2 Working mode and information unit**

000 - interface switched off

001 - 8N1 - ASCII

010 - 7E1 - ASCII

011 - 7O1 - ASCII

100 - 8N2 - RTU

101 - 8E1 - RTU

110 - 8O1 - RTU

111 - 8N1 - RTU

**Bit-1...0 Baud rate**

00 - 2400 bit/s

01 - 4800 bit/s

10 - 9600 bit/s

## **7. TECHNICAL DATA**

### **INPUTS:**

Input resistance:

- for voltage inputs  $> 4 \text{ M}\Omega$

- for inputs (5 mA and 20 mA)  $< 4 \Omega$

	Range	NA3-XXXXU	NA3-XXXXT	NA3-XXXXS	NA3-XXXXH
Pt100	(-200... +850)°C	X	X		
Pt500	(-200... +850)°C	X	X		
Pt1000	(-200... +850)°C	X	X		
J ( Fe-CuNi)	(-30... +1100)°C	X	X		
K (NiCr-NiAl)	(-50... +1370)°C	X	X		
N (NiCrSi-NiSi)	(-100... +1300)°C	X	X		
E (NiCr-CuNi)	(-20... +850)°C	X	X		
R (PtRh13-Pt)	(0... +1760)°C	X	X		
S (PtRh10-Pt)	(0... +1760)°C	X	X		
T (Cu-CuNi)	(-50... +400)°C	X	X		
Resistance measurement	0...400 $\Omega$	X	X		
Resistance measurement	0...4000 $\Omega$	X	X		
Voltage measurement	0...60 mV	X	X		
Voltage measurement	0...3 V	X			
Voltage measurement	0...10 V	X		X	
Current measurement	0...5 mA	X			
Current measurement	0...20 mA	X		X	
Voltage measurement	0...200 V	X			X
Voltage measurement	0...600 V	X			X
Current measurement	0...2 A	X			X
Current measurement	0...5 A	X			X

- for inputs (2 A and 5 A)  $10 \text{ m}\Omega \pm 10\%$

Intensity of current flowing through the resistance thermometer:  $< 170 \mu\text{A}$

Resistance of conductors linking the resistance thermometer with the meter:

$< 20 \Omega/1 \text{ wire}$

Thermocouple characteristics acc. EN 60584-1.

Resistance thermometer characteristics acc. IEC 751 + A1+A2.

#### OUTPUTS:

- **Analogue output** galvanically isolated, with a resolution = 0,025% of the range

- current programmable: 0/4..20mA      load resistance  $\leq 500 \Omega$
- or voltage programmable: 0..10V      load resistance  $\geq 500 \Omega$
- output response time                      100 ms
- output error                                  0.2 % of the range
- additional error due to ambient  
  temperature changes:                       $\pm (0.1\% \text{ of the range } / 10K)$

**– Relay output**

Relays (1 or 2); voltageless make contacts - maximal load:

- voltage                      250 V a.c., 150 V d.c.,
- current                      5 A 30 V d.c., 250 V a.c.,
- resistance load      1250 VA, 150 W.

Programmable alarm thresholds;

Three types of alarms;

Hysteresis defined by means of the lower and upper alarm threshold;

Signalling of alarm operation on the bargraph or by means of alarm diodes.

**– Output of open collector (OC) type**

voltageless, OC type with npn transistor (max. load 25 mA)

range of added voltage: 5...24 V d.c.

**– Digital output:**

- interface:                                      RS-485,
- transmission protocol:                      MODBUS,
- ASCII:    8N1, 7E1, 7O1,
- RTU:    8N2, 8E1, 8O1, 8N1,
- baud rate:                                        2400, 4800, 9600 baud
- maximal response time to the  
  request frame:                                300 ms.




**Memory parameters:**

- meter memory (record)                      750 samples
- min. record interval                          1 sec;

**Basic error:**                                      0.2%  $\pm 1$  digit

**Additional errors in nominal working conditions when measuring the temperature:**

- compensation of reference junction temperature changes	$\pm 0.2$ % of range
- compensation of wire resistance changes	$\pm 0.2$ % of range
<b>Additional error from ambient temperature changes</b>	$\pm (0.1$ % of range/10K)
<b>Averaging time</b>	min 500 ms, temperature measurement min 200 ms, other ranges
<b>Rated operation conditions:</b>	
- supply voltage depending on the execution code	95... <u>230</u> ...253 V a.c./d.c. 20... <u>24</u> ...40 V a.c./d.c.
- supply a.c. voltage frequency	40... <u>50/60</u> ...440 Hz
- ambient temperature	- 10... <u>23</u> ...55°C
- storage temperature	- 25...+85°C
- relative humidity	< 95% (no condensation)
- time of preliminary indicator heating	10 min
<b>Sustained overload:</b>	
- thermocouples, resistance thermometers	1 %
- measurement of voltage, current and resistance	10 %
<b>Momentary overload (3 s):</b>	
- sensor inputs and voltage 60 mV	30 V
- voltage input $\geq 3$ V	$10 \times U_n$ (< 1000 V)
- current input	$10 \times I_n$
<b>Readout field (depending on execution):</b>	4 seven-segment LED display, NA3-F digit height: 7 mm NA3-D digit height: 14 mm NA3-B without display indication range: -1999...9999  bargraph length: 82 mm (except NA3-D) - 45 segments in three-colour execution

	- 25 segments in seven-colour execution
	3 alarm diodes in NA3D execution
<b>Bargraph resolution</b>	programmable
<b>Bargraph accuracy</b>	± 0.5 segment
<b>Servicing:</b>	three keys:   
<b>Ensured protection degree (EN 60529):</b>	
- through the casing	IP 40
- from terminal side	IP 20
<b>Dimensions:</b>	96 x 24 x 125 mm (with terminals)
<b>Weight:</b>	< 0.3 kg
<b>Power consumption</b>	< 8 VA
<b>Resistance against supply decay</b>	acc. EN 61000-6-2:2002
<b>Electromagnetic compatibility:</b>	
- immunity	EN 61000-6-2:2002
- emission	EN 61000-6-4:2002
- additional error from electromagnetic risks	< 0.5%
<b>Safety requirements according EN 61010-1:</b>	
- installation category	III
- pollution degree	2
- phase-to-earth max. working voltage:	
input	600 V
supply	300 V
relays	300 V
analogue output	50 V
RS-485	50 V








## 8. BEFORE A FAILURE WILL BE DECLARED



In case of incorrect symptoms please to acquaint with the table below.

SYMPTOMS	PROCEDURE
1. Lack of indications on the display. The bargraph indicates nothing.	Check the connection of the feeder cable.
2. The time is displayed on the display, e.g. <b>H_12</b> alternately with <b>34:43</b> .	The number of measurements <b>Cnt</b> = 0 has been introduced. The meter is working in the SLEEP mode. It displays the current hour.
3. Marks  or  are displayed on the display.	Check the correctness of the input signal connection. See the service manual. Check also the setting of parameters <b>D_P</b> and <b>Ind</b> .
4. A signal inconsistent with our expectations occurs on the meter analogue output.	One must check if the load resistance of the analogue output is in accordance with technical data. Check if the individual characteristic is not switched on. In case of necessity make changes of individual characteristic parameters or introduce manufacturer parameters <b>Set</b> .
5. Lack of possibility to enter into the programming mode. The inscription <b>Err</b> is displayed.	The programming mode is protected by a password. When the user forgets which password has been introduced, he should contact by phone the manufacturer or the nearest authorised workshop.
6. Lack of certainty if all segments of the display or bargraph are efficient.	Enter into the programming matrix and switch the display and bargraph <b>tSt</b> test on. Character fields are lighted successively from 0000 to 9999. In the same time the bargraph is lighted with successive colours. If some of segments are not lighted or diodes have different colours, one must submit these defects to the nearest workshop.
7. During the operation in the programming mode, parameter values inconsistent with the range of changes given in the table 1, appear on the display.	Enter into the programming matrix and accept the <b>SEt</b> parameter. The meter will introduce values in accordance with the table 2.

8. A result inconsistent with our expectations appears on the display.	Check if the individual characteristic is not switched on. In case of necessity enter into the programming matrix and accept the <b>SEt</b> parameter. The meter will introduce parameters in accordance with the table 2.
9. The bargraph does not work in accordance with our expectations.	Check bargraph parameters. In case of a further incorrect operation, enter into the programming matrix and accept the parameter <b>SEt</b> . Switch the display and bargraph <b>tSt</b> test on.
10. Despite the exceeding of the alarm threshold the alarm relay does not switch on.	Check the delay of alarm operation introduced into the meter. In case of need, correct <b>dLY</b> parameters.
11. The meter, instead of displaying the measurement result, displays the parameter symbol and its value.	The meter is working in the preview mode or in the programming mode. Press the escape key  .
12. Despite of the introduced delay in the alarm operation, e.g. 30 seconds, the alarm after this time did not operate.	The lasting alarm state was shorter than the programmed, that means that during the lasting time, the alarm withdrawal state occurred. In such a case, the meter begins to count down the time from the beginning.
13. The meter does not establish the communication with the computer through the RS-485 interface.	Check if interface conductors ( <b>A, B, GND</b> ) were correctly connected. Then, check in the programming matrix the setting of the interface ( <b>bAud, trYb, Adr</b> ). These parameters must be the same as in the used software.

## 9. EXAMPLES OF NA3 METER PROGRAMMING

### Example 1. Programming of the individual characteristic.

If we want to programme so that to the value 4.00 mA will correspond the value 0 on the display, whereas, the value 20.00 mA will correspond to the value 100, one must:

- enter into the programming mode and choose the **D\_P** parameter responsible for the decimal point. Set the decimal point on **00000**
- choose the **Ind** parameter and switch the individual characteristic **On**
- choose the **I\_H1** parameter and introduce the value 4.00
- transit on the **d\_Y1** parameter and introduce the value 0

- transit on the **I\_H2** parameter and introduce the value 20.00
- transit on the **d\_Y2** parameter and introduce the value 100

### Example 2 Programming of an inverse individual characteristic.

If we want to programme so that to the value 4.00 mA will correspond the value 120.5 on the display, and to the value 20.00 mA, the value 10.8, one must:

- enter into the programming mode and choose the **D\_P** parameter responsible for the decimal point. Set the decimal point on **0000.0**
- choose the wybr c **Ind** parameter and switch the individual characteristic **On**
- choose the **I\_H1** parameter and introduce the value 4.00
- transit on the **d\_Y1** parameter and introduce the value 120.5
- transit on the **I\_H2** parameter and introduce the value 20.00
- transit on the **d\_Y2** parameter and introduce the value 10.8

### Example 3 Programming of the alarm with hysteresis

If we want to programme the alarm 1 operation so that at the value 850°C, this alarm will be switched on, whereas it will be switched off at the value 100°C, and the alarm 2 operation so that at the value 1000°C, this alarm will be switched off and switched on at the value -199°C, one must:

- enter into the programming mode , choose the **PrL** parameter of the alarm 1 and introduce the value 100
- transit on the **PrH** parameter of the alarm 1 and introduce the value 850
- transit on the **tYPA** parameter of the alarm 1 and choose select the function assigned as **nor**
- transit on the **tYPA** parameter of the alarm 2 and select the function **nor**
- choose the **PrL** parameter of the alarm 2 and introduce the value 1000
- transit on the **PrH** parameter of the alarm 2 and introduce the value -199

### Example 4 Programming of an alarm operating in a set interval with delay.

If we want that the alarm 1 will be switched on in the interval from 100 V to 300 V and operate only after 10 seconds, one must:

- enter into the programming mode , choose the **PrL** parameter of the alarm 1 and introduce the value 100
- transit on the **PrH** parameter of the alarm 1 and introduce the value 300
- transit on the **tYPA** parameter of the alarm 1 and select the function **On**
- transit on the **dLY** parameter of the alarm 1 and introduce the value 10.0

in case of the alarm state duration for a time longer than 10 seconds, the meter will switch the alarm relay on

### Example 5 Programming of an analogue output

If we want to programme so that the displayed value 0.00 mA for the channel 2 will correspond the value 4.00 on the analogue output, whereas to the value 20.00 mA , the value 20.00 mA, one must:

- enter into the programming mode, choose the **IndO** parameter and switch the individual characteristic **On**
- choose the **d\_H1** parameter and introduce the value 0.00
- transit on the **O\_Y1** parameter and introduce the value 4.00
- transit on the **d\_H2** parameter and introduce the value 20.00
- transit on the **O\_Y2** parameter and introduce the value 20.00

### Example 6 Programming of the recording every 20 seconds since 12:30:

- enter into the programming mode, choose the **Go\_r** parameter and introduce the value 12:30
- transit on the **IntE** parameter and introduce the value 00:00:20
- choose the **rEC** parameter and switch the recording **On**

After the exit from the programming matrix the memory will be erased and the meter will begin to record results since 12:30, every 20 seconds.

After the memory filling up, the recording will be switched off.

## 10. ORDERING PROCEDURE

Execution codes of NA3 meter (seeTable 5).

Table 5.

NA3 METER WITH BARGRAPH	X	X	X	X	X	X	X	X	XX	U
<b>Meter execution:</b>										
With bargraph and LED digital display .....	F									
With bargraph* .....	B									
With digital display.....	D									
<b>Bargraph colour (in case of D execution, write 0):</b>										
3-colour (R, G, R + G) .....	T									
7-colour (R, G, B, R+G, R+B, G+B, R+G+B).....	M									
<b>Display colour (in case of B execution, write 0):</b>										
red.....	R									
green.....	G									
blue.....	B									
<b>Input signal (table 6):</b>										
universal input .....	U									
temperature input**** .....	T									
standard input (10 V, 20 mA).....	S									
high signal input (200 V, 600 V, 2 A, 5 A).....	H									
on order** .....	X									
<b>Analogue output signal:</b>										
without analogue output .....	0									
current programmed, 0/4...20 mA .....	1									
voltage programmed, 0...10 V.....	2									
on order** .....	X									
<b>Additional outputs:</b>										
Without output* .....	0									
RS-485 digital output + 1 relay.....	1									
RS-485 digital output + 1 OC output .....	2									
2 relays* .....	3									
2 OC outputs* .....	4									
on order** .....	X									
<b>Supply:</b>										
95...253 V a.c./d.c. ....	1									
20... 40 V a.c./d.c. ....	2									
on order** .....	X									
<b>Kind of terminals:</b>										
socket - screw plug.....	0									
on order*** .....	X									
<b>Execution:</b>										
standard .....	00									
custom-made** .....	XX									
<b>Version:</b>										
standard .....	U									

\* In case of NA3 B X X X X (0, 3 or 4) complete the table 7.

\*\* After agreeing with the producer.

\*\*\* Possible execution with self-locking terminals.

\*\*\*\* Temperature input signal: Pt100, Pt500, Pt1000, resistance, thermocouple, voltage 0... 60 mV.

**Example of ordering:**Code: **NA3 F T R U 0 1 1 0 00 U** means:**F** - NA3 meter execution with a bargraph and a digital display,**T** - with three colours ( R, G, R+G),**R** - with a digital display, of red colour**U** - universal input (see table 6),**0** - without analogue output signal,**1** - RS-485 digital output + 1 relay,**1** - supply: 95...253 V a.c./d.c.,**0** - socket-screw plug terminals,**00** - standard execution,**U** - standard version.**In case of a custom-made execution or if you need some more additional technical information, please write to or phone our Export Department.**

Input signals

Table 6

<b>Universal input</b>	Resistance thermometer:	
	Pt100	(- 200... +850)°C
	Pt500	(- 200... +850)°C
	Pt1000	(- 200... +850)°C
	Thermocouple:	
	J ( Fe-CuNi)	(- 30... +1100)°C
	K (NiCr-NiAl)	(- 50... +1370)°C
	N (NiCrSi-NiSi)	(- 100... +1300)°C
	E (NiCr-CuNi)	(- 20... +850)°C
	R (PtRh13-Pt)	(0... +1760)°C
	S (PtRh10-Pt)	(0... +1760)°C
	T (Cu-CuNi)	(- 50... +400)°C
	Resistance	0... 400 Ω
	Resistance	0... 4000 Ω
	Voltage from shunt	0... 60 mV
	Voltage	0... 3 V
	Voltage	0... 10 V
	Voltage	0... 200 V
	Voltage	0... 600 V
	current	0... 5 mA
current	0... 20 mA	
current	0... 2 A	
current	0... 5 A	

Kind of output .....	<b>tYP</b>
Mathematical functions .....	<b>Func</b>
Kind of compensation .....	<b>Con</b>
Measurement averaging time .....	<b>Cnt</b>
Display characteristic .....	<b>Indi</b>
Measured value .....	<b>I_H1</b>
Displayed value .....	<b>d_Y1</b>
Measured value .....	<b>I_H2</b>
Displayed value .....	<b>d_Y2</b>
Bargraph type .....	<b>tYPb</b>
Bargraph colour .....	<b>coLr</b>
Bargraph lower threshold .....	<b>brL</b>
Bargraph higher threshold .....	<b>brH</b>
Alarming lower threshold .....	<b>PrL</b>
Alarming higher threshold .....	<b>PrH</b>
Alarm type .....	<b>tYPA</b>
Delay of alarm action .....	<b>dLY</b>
Support of alarm signalling .....	<b>HOLd</b>
Colour of the lower threshold alarm index .....	<b>CurL</b>
Colour of the higher threshold alarm index .....	<b>CurH</b>
Alarming lower threshold .....	<b>PrL</b>
Alarming higher threshold .....	<b>PrH</b>
Alarm type .....	<b>tYPA</b>
Delay of alarm action .....	<b>dLY</b>
Support of alarm signalling .....	<b>HOLd</b>
Colour of the lower threshold alarm index .....	<b>CurL</b>
Colour of the higher threshold alarm index .....	<b>CurH</b>
Alarming lower threshold .....	<b>PrL</b>
Alarming higher threshold .....	<b>PrH</b>
Alarm type .....	<b>tYPA</b>
Delay of alarm action .....	<b>dLY</b>
Support of alarm signalling .....	<b>HOLd</b>
Colour of the lower threshold alarm index .....	<b>CurL</b>
Colour of the higher threshold alarm index .....	<b>CurH</b>
Output characteristic .....	<b>IndO</b>
Displayed value .....	<b>d_H1</b>
Value on the analogue output .....	<b>O_Y1</b>
Displayed value .....	<b>d_H2</b>
Value on the analogue output .....	<b>O_Y2</b>
RS-485 baud rate .....	<b>bAud</b>
Kind of RS-485 transmission .....	<b>trYb</b>
Device address .....	<b>Adr</b>

## 11. MAINTENANCE AND GUARANTEE

The NA3 meter does not require any periodical maintenance. In case of some incorrect unit operations:

### **1. From the shipping date, during the period given in the annexed guarantee card**

One should take the meter down from the installation and return it to the Manufacturer's Quality Control Dept.

If the unit has been used in compliance with the instructions, the Manufacturer guarantees to repair it free of charge.

### **2. After the guarantee period:**

One should turn over the meter to repair in a certified service workshop.

The disassembling of the housing causes the cancellation of the granted guarantee.

Spare parts are available for the period of five years from the date of purchase.

**The Manufacturer policy is one of continuous improvement and we reserve the right to make changes in design and specification of any products as engineering advances or necessity requires and revise the above specification without notice.**











**Sifam Tinsley Instrumentation Inc**

3105, Creekside Village Drive, Suite 801

Kennesaw GA 30144

email – [psk@sifamtinsley.com](mailto:psk@sifamtinsley.com)

Phone - +1 404 736 4903